


SPI Electrical Validation and Protocol Decode Software

PGY-SPI Data Sheet

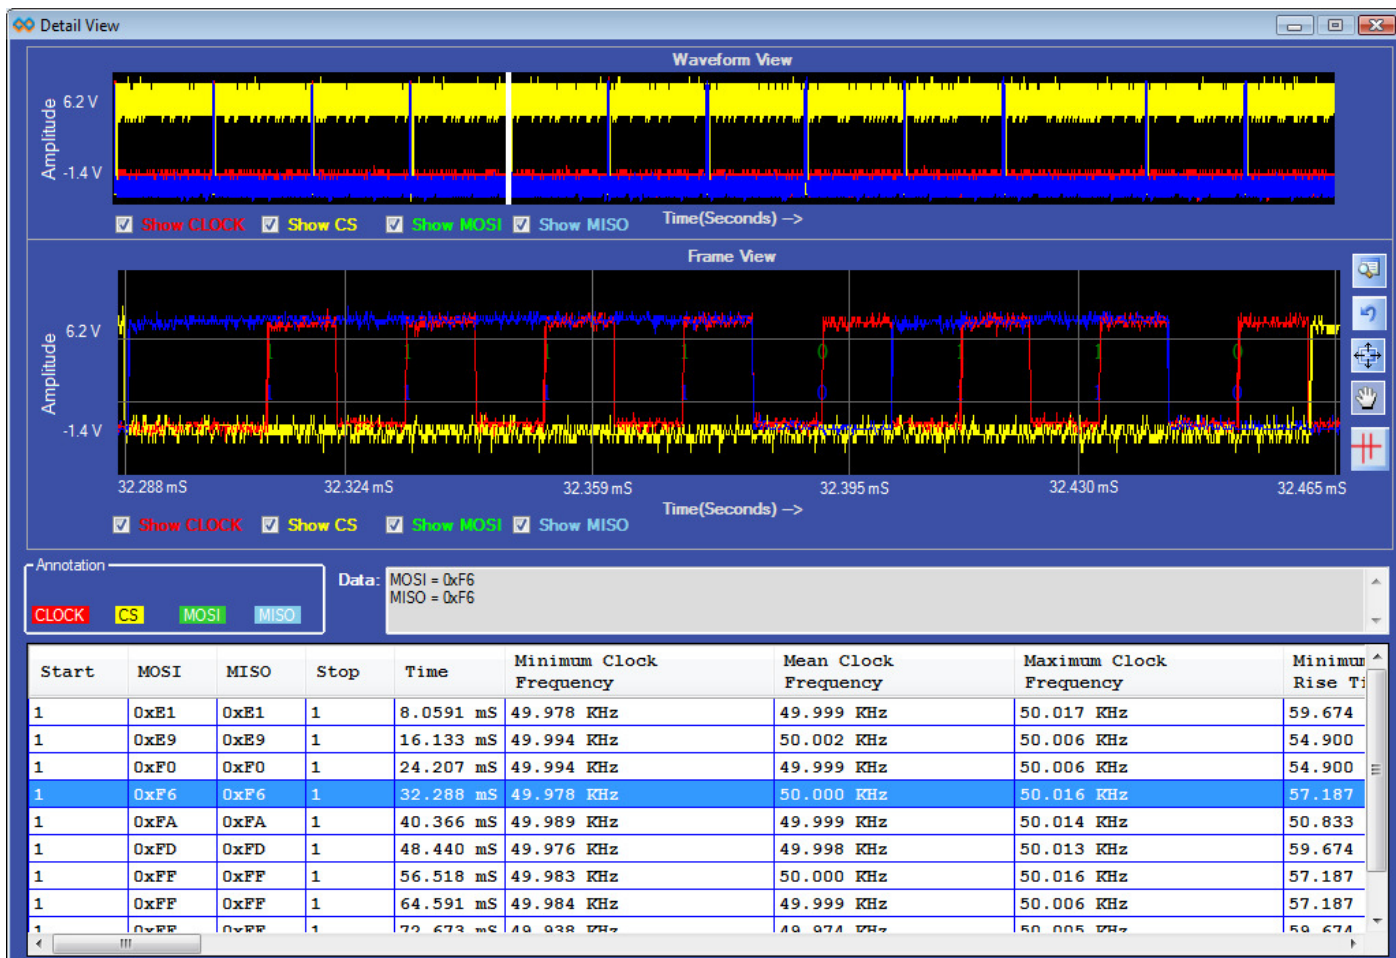


Engineers, designing and testing SPI hardware and firmware, need to measure electrical parameters and monitor protocol of SPI interface to ensure inter-operability. Engineers, test and debug their designs with easy-to-use instruments such as oscilloscopes to capture the electrical signals but use time-consuming and error prone tools to make electrical measurements and protocol analysis. Often, they need a single tool or instrument to cross-examine the protocol layer and the PHY layer to debug the designs to reduce development and testing cycles.

The PGY-SPI Electrical measurements and Protocol Decode Software offers electrical measurements and protocol decoding for SPI bus. This software provides the flexibility to set reference levels for electrical measurement and customised limits makes it most versatile solution to meet different needs of characterising SPI Signals. Now design and test engineers can automatically make accurate and reliable electrical measurements and decode protocols in PGY-SPI software using data acquired by Tektronix DPO5000, TDS7000, DPO/DSA/MSO7000 oscilloscope series to reduce the development and test cycle.

SPI Electrical Validation and Protocol Decode Software

PGY-SPI Data Sheet

Seamless Integration with Oscilloscope

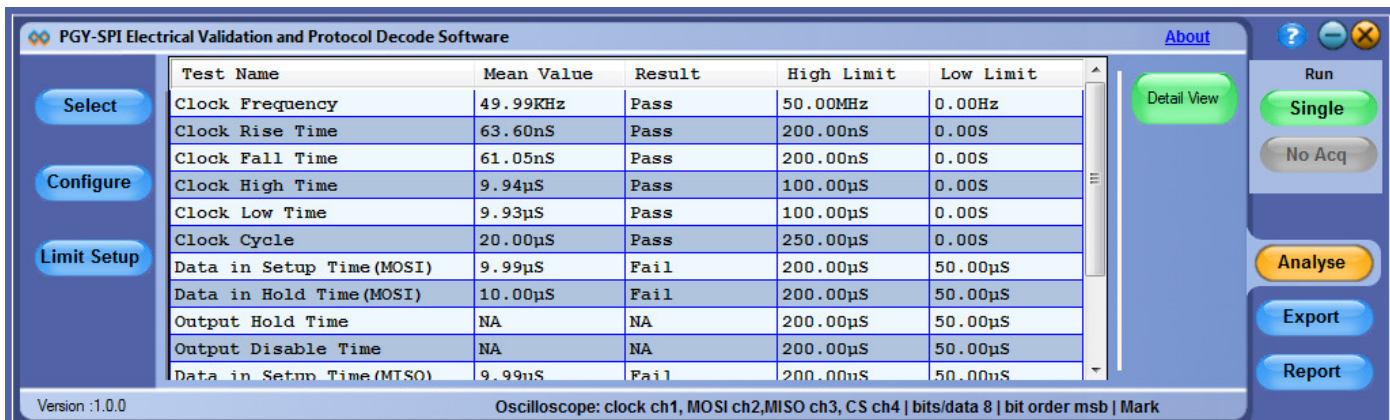


| Test Name | Mean Value | Result | High Limit | Low Limit |
|---------------------------|------------|--------|------------|-----------|
| Clock Frequency | 49.99KHz | Pass | 50.00MHz | 0.00Hz |
| Clock Rise Time | 63.60nS | Pass | 200.00nS | 0.00S |
| Clock Fall Time | 61.05nS | Pass | 200.00nS | 0.00S |
| Clock High Time | 9.94µS | Pass | 100.00µS | 0.00S |
| Clock Low Time | 9.93µS | Pass | 100.00µS | 0.00S |
| Clock Cycle | 20.00µS | Pass | 250.00µS | 0.00S |
| Data in Setup Time (MOSI) | 9.99µS | Fail | 200.00µS | 50.00µS |
| Data in Hold Time (MOSI) | 10.00µS | Fail | 200.00µS | 50.00µS |
| Output Hold Time | NA | NA | 200.00µS | 50.00µS |
| Output Disable Time | NA | NA | 200.00µS | 50.00µS |
| Data in Setup Time (MISO) | 9.99µS | Fail | 200.00µS | 50.00µS |

Version :1.0.0 Oscilloscope: clock ch1, MOSI ch2, MISO ch3, CS ch4 | bits/data 8 | bit order msb | Mark

PGY-SPI Software runs inside the Tektronix oscilloscopes and makes the electrical measurements, decodes protocols and displays the decoded data in a table, and links the decoded data to electrical signal in the waveform plot. SPI Protocol-based trigger can be set up using the built-in SPI trigger capabilities in Tektronix oscilloscopes.

Reference Level setup

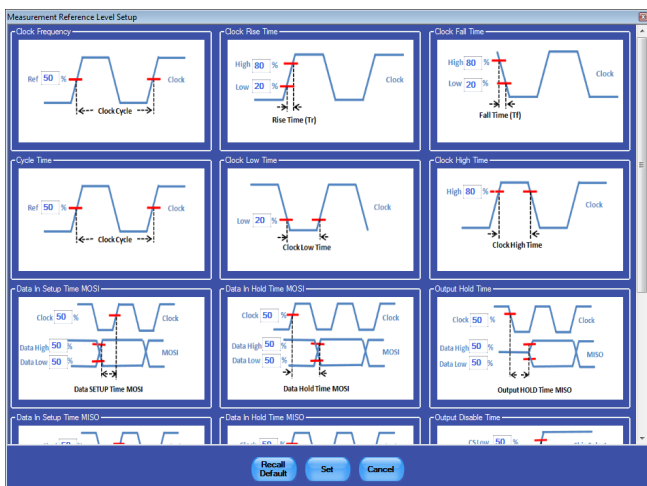

reference level setup to set measurement reference level of SPI signals. These limits are automatically applied while making selected SPI measurements in PGY-SPI software and reduces test time offering reliable measurements.

There are no standard measurements limits defined for SPI Bus for pass/fail test. The limits are varying in nature depending upon the SPI Bus speed. In order to characterise and validate SPI signals PGY-SPI software provides graphical measurement

SPI Electrical Validation and Protocol Decode Software

PGY-SPI Data Sheet

Characteristics:

| | | |
|-------------------------|---|-------------------------|
| Electrical Measurements | Clock Frequency | Data In Hold time MOSI |
| | Clock High Time | Output Disable Time |
| | Clock Low Time | Output Hold time |
| | Clock Rise Time | Data In Setup Time MISO |
| | Clock Fall Time | Data In Hold Time MISO |
| | Clock Cycle Time | |
| | Chip Select Deselect Time | Chip Select Hold Time |
| | Data in Setup Time MOSI | Chip Select Setup Time |
| Bus Speed | Custom; Limited by oscilloscope Bandwidth | |
| Protocol Decode | Hexadecimal, Octal, Binary, Decimal, ASCII | |
| Waveform window | Overlay of protocol decode data on waveform | |
| Report Generation | Customizable report in html format | |
| Export of data | CSV and Txt format | |

Features

- Automated electrical measurements with customizable reference level of SPI electrical signal.
- Automated measurements independent of speed of SPI Bus
- Customizable measurement limit setup for pass/fail validation of electrical signal to enable measurements at different data speed.
- Decodes SPI signals MOSI and MISO for easy understanding of protocol
- Links the protocol content to the electrical signal in the oscilloscope for easy understanding of the electrical characteristics of the protocol
- Overlays the protocol data on analog waveform in a waveform plot window
- Zooms the selected SPI packet content in the decode table in the waveform plot waveform window for easy analysis of electrical characteristics of the I2C frame
- Ability to view protocol decode data in hexadecimal, decimal, binary, octal, and ASCII formats
- Ability to store the SPI protocol data in CSV and txt format
- Utility features like zoom, undo, and fit screen for easy debugging while correlating the protocol data to the waveform
- Report generation in html format
- Supports wfm and isf file formats for offline analysis

SPI Electrical Validation and Protocol Decode Software

PGY-SPI Data Sheet

Oscilloscopes Supported

The following Tektronix oscilloscopes are supported:

- DPO5000 Series
- DPO7000 Series
- DPO/MSO/DSA 70000 Series

Ordering Information

PGY-SPI Electrical Validation and Protocol Decode Software (shipment includes CD with PGY-SPI software and license key)

About Prodigy Technovations Pvt Ltd

Prodigy Technovations Pvt Ltd (www.prodigytechno.com) is a leading global technology provider of Protocol Decode, and PHY layer testing solutions on test and measurement equipment. The company's ongoing efforts include successful implementation of innovative and comprehensive protocol decode and PHY Layer testing solutions that span the serial data, telecommunications, automotive, and defence electronics sectors worldwide.

Contacts:

Prodigy Technovations Pvt. Ltd.; 4123, 6th Cross, 19th Main, HAL II Stage, Indiranagar, Bangalore, India 560008

Phone number: +91 80 32553020/ +91 9880027949; Email: contact@prodigytechno.com

Other products

- HDMI/MHL Protocol Compliance Test Software
- I2C Electrical validation and Protocol Decode Software
- SPI Protocol Analysis Software
- UART/RS232 Protocol Decode Solution
- FlexRay Protocol and SI Analysis Software
- I2S Electrical, Audio, and Protocol Testing Software
- USB2.0 Protocol Decode Software